



Installation Guide

MOBOTIX c ONE NurseAssist *powered by Kepler Vision Technologies*

© 2026 MOBOTIX AG



Table of Contents

Table of Contents	2
Before You Start	5
Support	6
MOBOTIX Support	6
MOBOTIX eCampus	6
MOBOTIX Community	6
Legal Notes	6
Protective Measures	8
Notes on Cabling	8
Fire Protection	8
Lightning and Surge Protection	8
Drilling Template	9
Drilling Template PDF	10
c ONE: Scope of Delivery	12
Mounting Supplies: Scope of Delivery	13
Overview	15
Sensor Side	16
Back Side	16
Technical Specifications	17
Order Information	18
Hardware	18
Image and Video Properties	20
Kepler NurseAssist App - Specifications	20
General Software Features	23
Further Video Analysis	24
Nurse Call Systems / Video Management Software	24
Dimensions	25
Mounting	27
Before Mounting the Camera	28
Removing the Back Plate	28
Attaching the Back Plate	29
Connecting the Camera	30
Connecting a USB-C Device	30
Connecting I/O Devices	31
I/O Terminal Pin-Out	31
Connecting the Camera to the Network	32
Mounting Options	33
Flush Ceiling Installation	33
Removing the Camera from the Ceiling	34
Surface Ceiling Installation	34
Preparing the Camera	35
Preparing the On-Wall Mounting Set	35
Installing the On-Wall Mounting Set	36
Removing the Camera	38
Adjusting the Camera Lens	39
Adjusting and Focusing the Camera Lens	39
Operating the Camera	41
Getting Started	42
LED States	42

Network Settings	42
Initial Camera Setup	42
Check the Preconditions	42
Access the Camera	43
Find the "Real" IP Address of the Camera	46
Automatic Setup using MxManagementCenter	46
Network Settings on the Camera in MxMC	46
Network Settings on the Camera in the Web Browser	48
Camera Software in the Browser	49
Access the Camera in the Web Browser	50
Basic Settings	50
Maintenance	53
Replacing the microSD Card	54
Cleaning the Camera	54
Cleaning and Disinfection Instructions	55
General Requirements	55
Cleaning Procedure	55
Post-Cleaning Requirements	56
Approved Cleaning Agents and Disinfectants	56
Incompatible Cleaning Agents	56

Before You Start

Support	6
Legal Notes	6
Protective Measures	8

Support

MOBOTIX Support

If you need technical support, please contact your MOBOTIX dealer. If your dealer cannot help you, he will contact the support channel to get an answer for you as quickly as possible.

If you have internet access, you can open the MOBOTIX help desk to find additional information and software updates.

Please visit www.mobotix.com > Services > Help Desk.



MOBOTIX eCampus

The MOBOTIX eCampus is a complete e-learning platform. It lets you decide when and where you want to view and process your training seminar content. Simply open the site in your browser and select the desired training seminar.

Please visit www.mobotix.com/ecampus-mobotix.



MOBOTIX Community

The MOBOTIX community is another valuable source of information. MOBOTIX staff and other users are sharing their information, and so can you.

Please visit community.mobotix.com.



Legal Notes

This document and its contents are the property of MOBOTIX AG and are protected by applicable copyright laws. Any reproduction, distribution, modification, or use of this document, in whole or in part, without prior written permission of MOBOTIX AG is strictly prohibited.

All product names, trademarks, logos, and brands referenced in this document are the property of their respective owners. These may include, but are not limited to, trademarks and certification marks of third-party organizations. The use

of such marks is for identification and informational purposes only and does not imply any affiliation with or endorsement by the respective trademark owners. MOBOTIX AG acknowledges the rights of all trademark holders and makes no claim to trademarks owned by third parties.

Legal Aspects of Video and Sound Recording

You must comply with all data protection regulations for video and sound monitoring when using MOBOTIX AG products. Depending on national laws and the installation location of the cameras, the recording of video and sound data may be subject to special documentation or it may be prohibited. All users of MOBOTIX products are therefore required to familiarize themselves with all applicable regulations and to comply with these laws. MOBOTIX AG is not liable for any illegal use of its products.

Declaration of Conformity

The products of MOBOTIX AG are certified according to the applicable regulations of the EC and other countries. You can find the declarations of conformity for the products of MOBOTIX AG on www.mobotix.com under **Services > Download Center > Marketing & Documentation > Certificates & Declarations of Conformity**.

RoHS Declaration

The products of MOBOTIX AG are in full compliance with European Unions Restrictions of the Use of Certain Hazardous Substances in Electrical and Electronic Equipment (RoHS Directive 2011/65/EU) as far as they are subject to these regulations (for the RoHS Declaration of MOBOTIX, please see www.mobotix.com, **Services > Download Center > Marketing & Documentation > Brochures & Guides > Certificates**).

Disposal

Electrical and electronic products contain many valuable materials. For this reason, we recommend that you dispose of MOBOTIX products at the end of their service life in accordance with all legal requirements and regulations (or deposit these products at a municipal collection center). MOBOTIX products must not be disposed of in household waste! If the product contains a battery, please dispose of the battery separately (the corresponding product manuals contain specific directions if the product contains a battery).

Disclaimer

MOBOTIX AG does not assume any responsibility for damages, which are the result of improper use or failure to comply to the manuals or the applicable rules and regulations. Our General Terms and Conditions apply. You can download the current version of the **General Terms and Conditions** from our website at www.mobotix.com by clicking on the corresponding link at the bottom of every page.

FCC Disclaimer

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

Protective Measures

WARNING!

When laying cables indoors and outdoors, the current regulations for cable laying, lightning and fire protection must always be observed.

MOBOTIX cameras and devices are protected against the effects of minor over voltages by a number of measures. However, these measures cannot prevent larger surge voltages from causing damage to the camera. When installing the cameras outdoors, special attention should therefore be paid to lightning protection and the associated dangers for the building and network infrastructure.

In general, you should only have MOBOTIX cameras and devices installed by certified specialist companies that are familiar with the installation and safe operation of network devices and the underlying regulations for lightning and fire protection as well as the current technology for preventing damage from surge voltages.

Notes on Cabling

- **Data cable:** Only double-shielded CAT5 cable or better (S/STP) may be used as data cable for the Ethernet interface.
- **Cable length:** The individual cable sections must not exceed the maximum permissible lengths in order to ensure perfect data transmission.
- **Avoidance of induction:** Data cables may only be laid parallel to power or high-voltage lines if the prescribed minimum distances are observed.

Fire Protection

When laying cables for the power supply, the relevant country-specific regulations (e.g. VDE in Germany) and the fire protection regulations valid at the installation site must be observed.

Lightning and Surge Protection

Measures should always be taken to protect this device from electrical surge damage.


Further information on how to avoid damage caused by lightning and over voltage is available from manufacturers of lightning and over voltage protection devices.

Drilling Template

Open this file in a PDF viewer (Adobe Reader or similar) and print the file **without scaling (original size)**.

NOTE!

Drilling template: www.mobotix.com > [Services](#) > [Download Center](#) > [Marketing & Documentation](#) > [Drilling Templates](#).

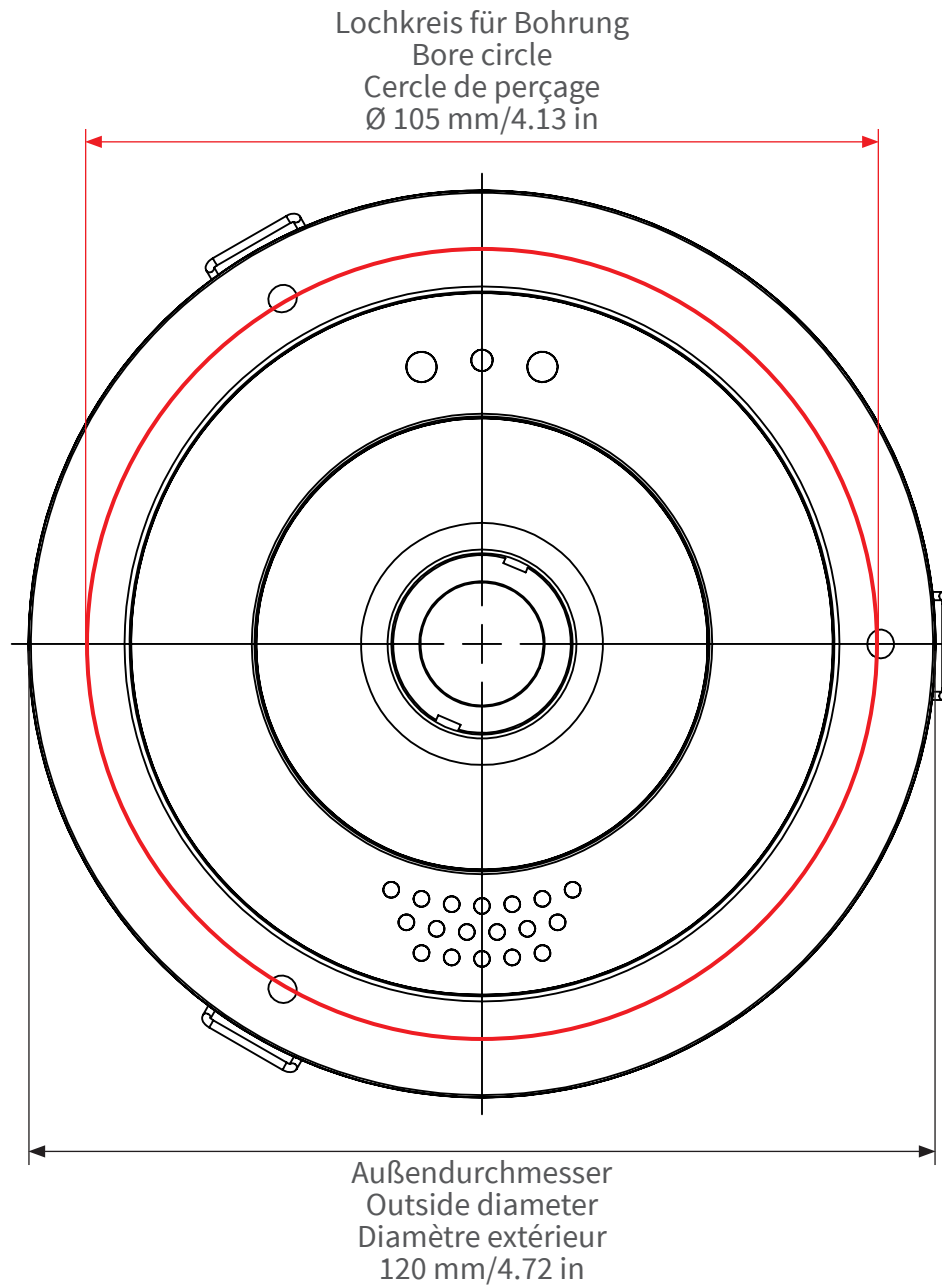

Nur in Originalgröße
kopieren oder ausdrucken!
Always copy or print at 100%
of original size!
Copier ou imprimer
uniquement aux dimensions
d'origine !

2

c ONE: Scope of Delivery	12
Mounting Supplies: Scope of Delivery	13


c ONE: Scope of Delivery



Scope of delivery c ONE: Body

Item	Count	Description
1.1	1	c ONE
1.2	1	MOBOTIX Ethernet patch cable, 50 cm/19.7 in (installed)
1.3	1	SD card 64 GB (installed)
1.4	1	Detachable I/O terminal block
1.5	1	Mounting supplies (see Scope of Delivery c ONE: Mounting Supplies, p. 13)
1.6	1	Safety Information
1.7	1	Sticker with IP address of camera

Mounting Supplies: Scope of Delivery

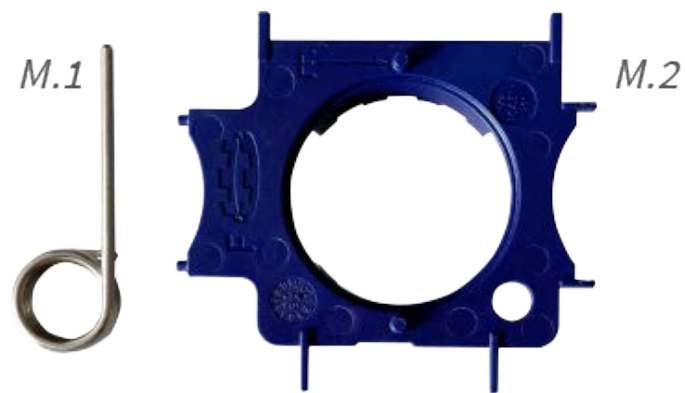


Scope of Delivery c ONE: Mounting Supplies

Item	Count	Description
M.1	1	Disassembly tool
M.2	1	MultiTool module wrench


Overview

Sensor Side	16
Back Side	16

Sensor Side

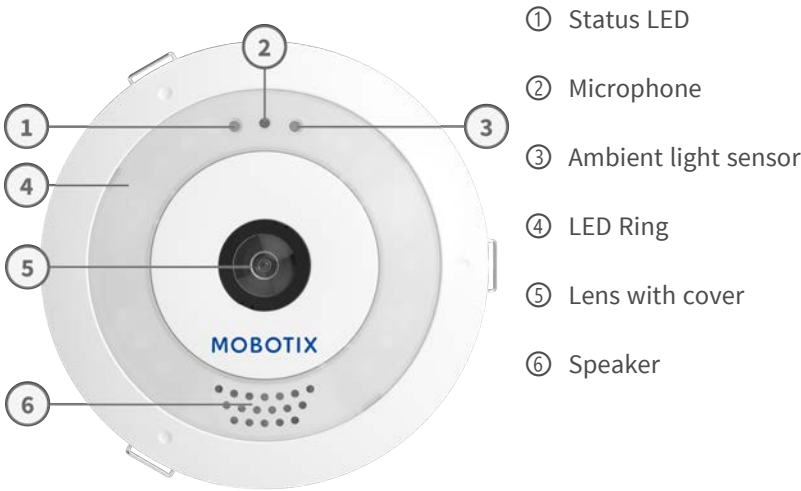

Back Side

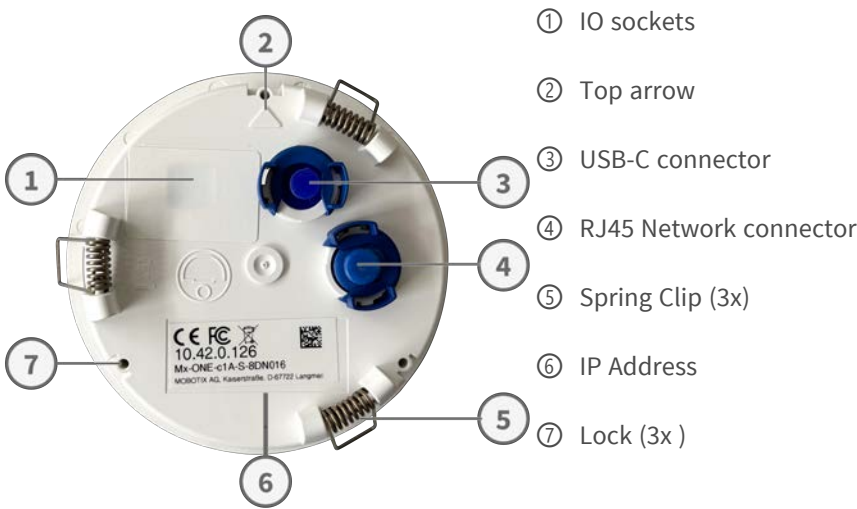

Technical Specifications

Order Information	18
Hardware	18
Image and Video Properties	20
Kepler NurseAssist App - Specifications	20
General Software Features	23
Further Video Analysis	24
Nurse Call Systems / Video Management Software	24
Dimensions	25

Order Information

Name	MOBOTIX c ONE NurseAssist <i>powered by Kepler Vision Technologies</i>
Order Code:	Mx-ONE-c1A-S-NurseAssist
NOTE! This order code covers the NurseAssist sensor hardware only. Analytics functionality requires a separate subscription license (Basic, Extended, or Lying Position).	

Hardware

Feature	Properties
Image sensor (DN)	4K (1:1) effective max. resolution 2160x2160
Light sensitivity	Day Mode (Color): 0,1 lx @ 1/60 s; 0,005 lx @ 1 s Night Mode (B/W): 0,02 lx @ 1/60 s; 0,001 lx @ 1 s
Exposure control	Manual and automatic mode 1 s to 1/16,000 s
IP / NEMA protection class	IP40
Intended use	Not intended for use in hazardous areas (Ex areas)
Operating temperature range	-20 to 40 °C/-4 to 104 °F
Internal DVR Storage	Internal microSD card (SDHC/SDXC), 64 GB out-of-the-box, max. 2 TB.
Allowed cable dimensions for cables connected to the PCB terminals	<i>Conductor cross section</i> AWG20 - 26 Rigid0.14mm ² - 0.5mm ² Flexible0.14mm ² - 0.5mm ² Flexible with ferrule0.25mm ² - 0.34mm ²
Input	Contact Closure (no galvanic isolation necessary) or up to 30 Vrms AC / 50V DC Switching thresholds - Input >1.6 V results in detected HIGH - Input <0.9 V results in detected LOW (after a HIGH) Max. length for cables: 50m
Output	1x dry contact, form A (max 30 Vrms / max, 50V DC/ 60 W/ 2A DC)

Feature	Properties
Microphone/Speaker	Integrated microphone: ■ Sensitivity: -35 dB +/-4 dB (0 dB = 1 V/pa, 1 kHz) Integrated speaker: ■ 0.9 W at 8 Ohm 1 external speaker optional
Integrated illumination	IR LEDs, 850 nm, up to 25 m²/269 ft² (may be more depending on scene) White light for emergency lighting
Tampering Detection	Integrated Shock Sensor
Max. power consumption	12.95 W
Electrical surge protection	via Overvoltage Protection Box (not part of the scope of delivery)
PoE standard	PoE (802.3af-2003) / Class 3
Interfaces	■ Ethernet 1000BaseT (RJ45 according to EIA/TIA-568B) ■ USB-C / USB 2.0 High Speed Power Output 5.1 V / 0.9 A / 4.5 W ■ 12-24 V DC power supply ■ Digital I/O: 1 Input / 1 Output
Status LED	multicolor (7 color)
Mounting Options	In-ceiling mountable; on-wall via optional accessories
Dimensions (Ø x height)	120 x 54 mm/4.72 x 2.13 in
Weight	360 g
Housing	PBT-30GF
Standard accessories	
Detailed technical documentation	www.mobotix.com > Services > Download Center > Marketing & Documentation
MTBF	100,000 hours
Certificates	EN 55032, EN 55035, EN 61000-6-1, EN 61000-6-2, EN 61000-6-3, EN 61000-6-4, EN 62368-1, EN 63000, AS/NZS CISPR32, 47 CFR Part 15b, NRTL
Protocols	DHCP (client and server), DNS, ICMP, IGMP v3, IPv4, IPv6, HTTP, HTTPS, FTP, FTPS, NFS, NTP (client and server), MQTT, RTP, RTCP, RTSP, SFTP, SIP (client and server), SMB/CIFS, SNMP, SMTP, SSL/TLS 1.3, TCP, UDP, VLAN, VPN, Zeroconf/mDNS
Manufacturer warranty	5 years

Image and Video Properties

Feature	Properties
Available video codecs	H.264, H.265, MxPEG+, MJPEG
Image resolutions	CIF (320x240; 4:3), nHD ² (360x360; 1:1), nHD (640x360; 16:9), VGA (640x480; 4:3), SVGA (800x600; 4:3), XGA (1024x768; 4:3), HD ² (720x720; 1:1), HD (1280x720; 16:9), Mega (1280x960; 4:3), FullHD ² (1080x1080; 1:1), FullHD (1920x1080; 16:9), QXGA (2048x1536; 4:3), UltraHD ² (2160x2160; 1:1), Custom Size
Multi streaming	H.264, H.265 with triple streaming
Multicast stream via RTSP	Yes
Max. frame rate	MxPEG: 20@4K, H.264: 30@4K, H.265: 30@4K

Kepler NurseAssist App - Specifications

General

Product Name	Kepler NurseAssist App
Order Code	Basic Starter: Mx-ONE-APP-KEP-NUA-1S/ -2S/ -3S/ -4S/ -5S Extended: Mx-ONE-APP-KEP-NUA-EXT-1/ -2/ -3/ -4/ -5 Lying Position: Mx-ONE-APP-KEP-NUA-LPO-1/ -2/ -3/ -4/ -5
Supported MOBOTIX Cameras	c ONE NurseAssist
Minimum Camera Firmware	v8.2.x.x
MxManagementCenter compatibility	- min. MxMC v2.9.x - Event Search: Smart Data Interface license included

NurseAssist Software Features According to License Tiers

NurseAssist Basic

- monitoring of the well-being of patients in private rooms, corridors and common areas of Healthcare facilities.
- minimization of reaction times due to decentralized state-of-the-art fall detection.
- prevention of accidents through person down, person in bed and person out of bed event.
- automatized detection and localization of the bed in the patient's room.
- GDPR compliant operation through event-controlled obscuring of live and recorded images.
- Dynamic masking of a person in bed as additional privacy protection measure.
- Continuous monitoring of sensor functions and analysis processes with the help of the App Heartbeat
- * IP-based bidirectional communication via integrated microphone and speaker
- * Noise level analysis enables the detection of loud ambient noise (e.g., loud shouting).
- Integrated shock detector for detecting physical tampering or vibrations
- Additional device health monitoring functions, including connectivity and uptime monitoring
- Configurable system status display via sensor status LED
- REST API interface enables deep integration and remote control of all sensor functions

NOTE!

*The sensor's audio functions are disabled by default and are enabled by an authorized administrator if required.

NurseAssist Extended

Plug-In license required to extend the NurseAssist status and alarm notifications with the following functions:

- Person is getting up from bed
- Person sits on the edge of the bed
- Person is getting up from a chair
- Person has entered the bathroom / is in the bathroom
- Person has left the room
- Person has entered the room
- Bed is not recognized / is not present
- Distinction between person lying and sitting on the floor

NOTE!

The Plug-In license requires MOBOTIX NurseAssist Smart Sensor or licensed Kepler NurseAssist Certified App.

Technical Specifications

Kepler NurseAssist App - Specifications

NurseAssist Lying Position	License to extend the NurseAssist Basic status and alarm notifications with the following functions: ■ Continuous monitoring of a person's lying position in bed (e.g., back, left side, right side) ■ Monitoring of prolonged stay in the same position ■ Notification if a person has not changed it's lying position for a defined period of time ■ Support for individualized care plans and decubitus prevention routines ■ Integration into existing alarm logic and reporting
----------------------------	---

Scene Requirements

Room size	max. 25m ² assuming an almost square room (e.g. 5x5 m) by radius of 4 m - long and narrow rooms will not work.
Required installation position (camera)	ceiling-mounted
Recommended installation height (camera)	2.0m - 3.5m
Mounting distance from bed	0.5m - 3.0m
Mounting distance from wall	> 70cm

General Software Features

Feature	Properties
WDR	Up to 120 dB
Software features	■ H.264, H.265 Multistreaming ■ Multicast stream via RTSP ■ Digital pan, tilt, zoom/vPTZ (up to 8x zoom) ■ Genetec protocol integration ■ Programmable exposure zones ■ Snapshot recording (pre/post-alarm images) ■ Continuous recording ■ Event recording ■ Time-controlled flexible event logic ■ Weekly schedules for recordings and actions ■ Event video and image transfer via FTP and email ■ Playback and QuadView via web browser ■ Animated logos on the image ■ Master/Slave functionality ■ Privacy zone scheduling ■ Remote alarm notification (network message) ■ Programming interface (HTTP API) ■ MxMessageSystem ■ MQTT (Message Queuing Telemetry Transport)
ONVIF compatibility	Profile G, S, T
Master/Slave functionality	Yes
Remote alarm notification	Email, MQTT, MxMessageSystem, network message (HTTP/HTTPS), SNMP, SIP
DVR/image storage management	■ On internal microSD card ■ On external USB and NAS devices ■ Different streams for live image and recording ■ MxFFS with buffered archive, pre- and post-alarm images, storage monitoring with error reporting
Camera and data security	FIPS 140-3 validated encryption (OpenSSL 3.1.2, NIST CMVP #4985), VPN with FIPS-certified library, HTTPS with custom X.509 certificates (TLS), AES encryption at rest (microSD / NAS), role-based access control, IP-level access control list, audit trail / web server access log, intrusion detection with automatic IP lockout, IEEE 802.1X port-based network access control, digital image signature
Firmware Tampering Detection	Digital Signature

Further Video Analysis

Feature	Properties
Video motion detection	Yes
MxActivitySensor	Version 1.0, 2.1

Nurse Call Systems / Video Management Software

Feature	Properties
3rd Party Nurse Call Systems	Extensively integrated; documented integrations available at: community.mobotix.com > MOBOTIX 7 Certified Apps > Kepler NurseAssist
MOBOTIX HUB	Supported, compatible with MOBOTIX HUB NurseAssist Dashboard www.mobotix.com > Services > Download Center > Software Downloads
MxManagementCenter	Yes (latest version recommended) www.mobotix.com > Services > Download Center > Software Downloads
MOBOTIX LIVE App	Yes (available in Google Play Store (Android) and Apple App Store (iOS)).
3rd Party VMS Software	See ONVIF Profile S, T and G specification

Dimensions

NOTE!

Drilling template: www.mobotix.com > Services > Download Center > Marketing & Documentation > Drilling Templates.

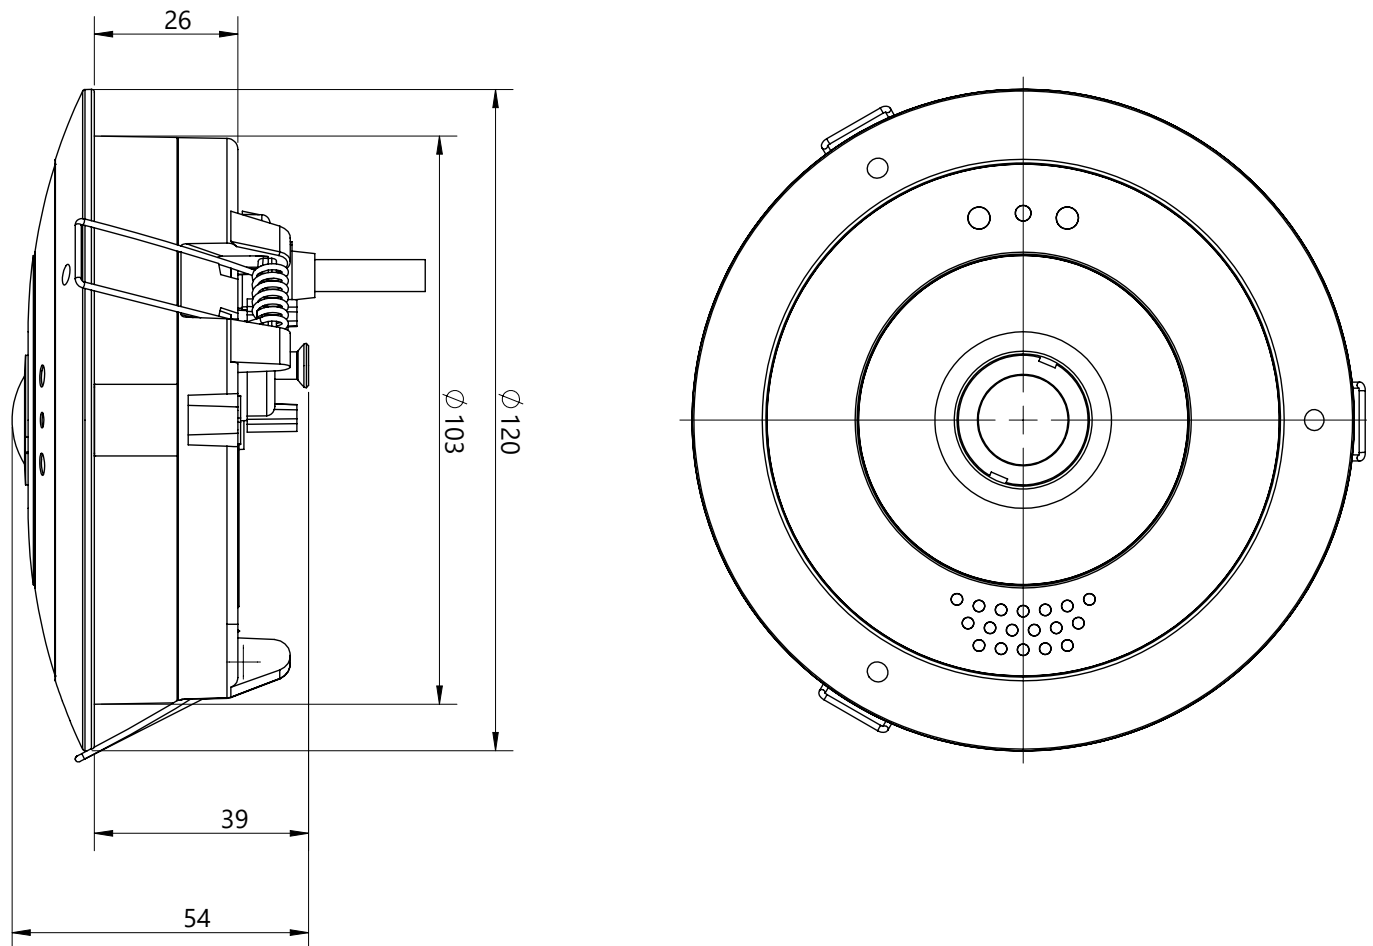


Fig. 1: MOBOTIX c ONE: All measurements in mm

Mounting

Before Mounting the Camera	28
Removing the Back Plate	28
Attaching the Back Plate	29
Connecting the Camera	30
Mounting Options	33
Adjusting the Camera Lens	39

Before Mounting the Camera

NOTE!

You will need the camera's IP address to access the camera in the network (see [Camera Software in the Browser](#), p. 49).

Before mounting the camera make sure to copy the IP address ① from the back side of the camera housing (see [Back Side](#), p. 16) or on the camera packaging.

The MOBOTIX c ONE is primarily designed for ceiling mounting. With the appropriate accessories, it can be mounted in a corner, on a pole, or in other mounting positions.

- Ceiling mounting (see [Flush Ceiling Installation](#), p. 33)

NOTE!

Drilling template: www.mobotix.com > [Services](#) > [Download Center](#) > [Marketing & Documentation](#) > [Drilling Templates](#).

Before mounting the MOBOTIX c ONE, the following questions should be answered:

- Where and how will the camera be mounted?
- How is the mounting surface level?
- Which other mounting options are available?
- Which accessories might be needed?
- How is the camera connected to the network and how is the power supplied?
- How are the connections furnished from the building?
- What cabling considerations are necessary?
- Do you want to use a larger SD card (see [Replacing the microSD Card](#), p. 54)?

The following sections will answer these questions. If you have further questions, please ask your MOBOTIX partner or contact the MOBOTIX support under www.mobotix.com > [Services](#) > [Help Desk](#).

Removing the Back Plate


The following tasks require opening the camera housing:

- [Replacing the microSD Card](#), p. 54.


1. In order to remove the back plate, you will need to push the delivered disassembly tool [Mounting Supplies: Scope of Delivery, p. 13](#), into the three holes on the back one after the other to release the locking tabs (see red circles in figure).



2. Insert the disassembly tool into a hole and press firmly until you feel a stop ① .

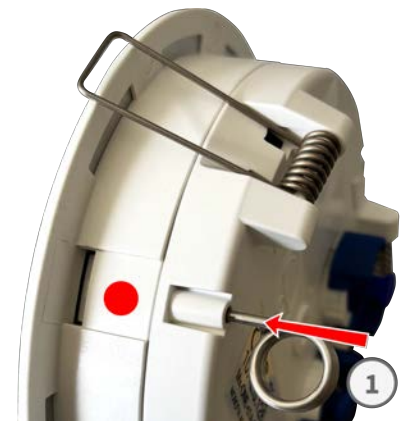

3. Gently push against the nearest spring clip to push the lock out of its seat and to lift the back plate from the housing ② . Repeat the process for the two other locks.
4. Lift the housing cover off the camera housing.

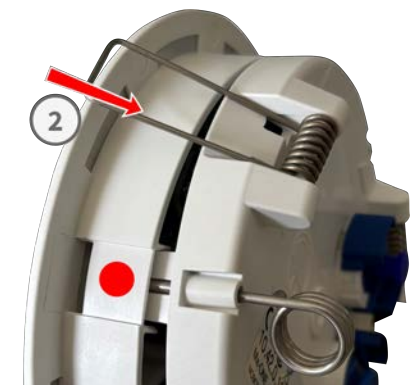

Attaching the Back Plate


CAUTION!

Before attaching the back plate, make sure that the SD card is properly locked in place, since the card can be damaged otherwise.

Mounting

Connecting the Camera

1. Position the upper locking tab (marked with an arrow on the housing cover) above the SD card. Then gently press the back plate into position until all three locking tabs click into place.

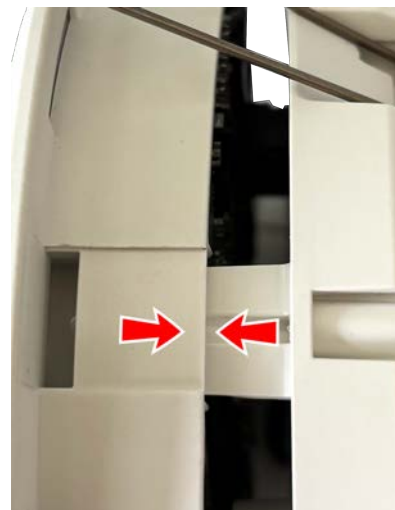

Connecting the Camera

All connections to the camera (network, USB-C, inputs/outputs) can be made directly on the camera. No further accessories are required for this. A PoE switch provides the camera's power supply.

Connecting a USB-C Device

The camera has a USB-C port that allows connecting external storage media or extension boxes, for example.

1. To access the USB-C port, open the blue bayonet catch ① of the plug lock by turning it away from the sealing plug, then remove the sealing plug.



2. Plug the USB-cable into the USB connector so that the small lug plug fits into the USB connector.
3. Attach bayonet catch.
4. Connect the USB-C device to the USB cable.



Connecting I/O Devices

The MOBOTIX c ONE has an I/O terminal that allows connecting multiple I/O devices.

I/O Terminal Pin-Out




In + Out + Spk + DC +

In - Out - Spk - DC -

CAUTION!

Before you proceed pay attention to the intended use or polarity of the slots. Ensure that the connections are assigned correctly as shown in the overview diagram above.


1. On the back of the camera, remove the sticker ① covering the I/O terminal block connector.

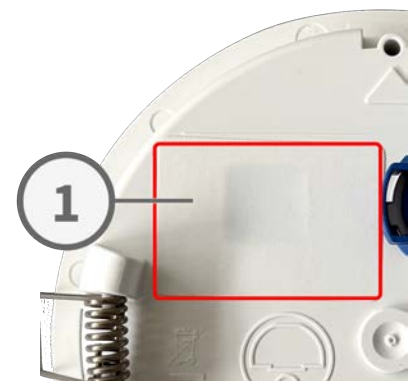

Mounting

Connecting the Camera

2. Press the I/O terminal block ② into the I/O connector until it is fully seated.

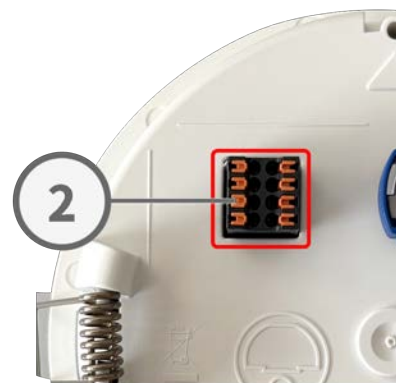

3. Strip 5 mm of insulation from the ends of the connection wires of the I/O devices, plug them in the respective units into the corresponding slots ② (see [I/O Terminal Pin-Out, p. 31](#)) of the connection terminal and check their tight fit.



Connecting the Camera to the Network

CAUTION!

- The PoE switch must provide Class 4 according to PoE (802.3af-2003) / Class 3 as well as the 100/1000 Mbps Ethernet interface of the camera.
- It is highly recommended to use an uninterruptible power supply (UPS) for the switch.
- The maximum length of the network cable for remotely supplying power is 100 m (300 ft).

1. **NOTE!**

It's recommended to connect the camera with the MX-Overvoltage-Protection-Box (RJ45 or LSA). This ensures a weatherproof (IP66) network and power connection network connector with surge protection of up to 4 kV (refer to the corresponding manual from the MOBOTIX website www.mobotix.com > **Services** > **Download Center** > **Marketing & Documentation**).

Mounting Options

The camera can be installed flush-mounted in a suspended ceiling without additional accessories. Alternatively, it can be installed on a ceiling or in a corner using the MOBOTIX On-Wall Mounting Set or Corner Mounting Set, both available as optional accessories.

NOTE!

Before mounting the camera

- Determine the optimal installation position and ensure that the field of view is not obstructed. After installation, you can fine-tune the image.
- Ensure that a PoE power supply compliant with PoE (802.3af-2003) / Class 3 is available at the installation location.

Flush Ceiling Installation


1. Use the drilling template or draw a circle with 105 mm/4.13 in diameter for the cut-out ① (see [Drilling Template, p. 9](#)).
2. Cut out the hole for the camera, then guide the Ethernet cable and any other cables you want to attach to the camera through the hole.
3. Insert the cables into the appropriate connectors and fasten them using the blue bayonet catches (see [Back Side, p. 16](#)).



Mounting

Mounting Options

4. Make sure that the camera points into the desired direction: The arrow icon on the back shows the "up" direction of the image.
5. Press the spring clips back and insert the camera into the hole for the camera. The spring clips will snap outwards, thus firmly holding the camera in place.
6. Make sure that you only press back the spring clips as shown on the right ②. Do not press them back any further as the springs may snap out of their fixtures otherwise.

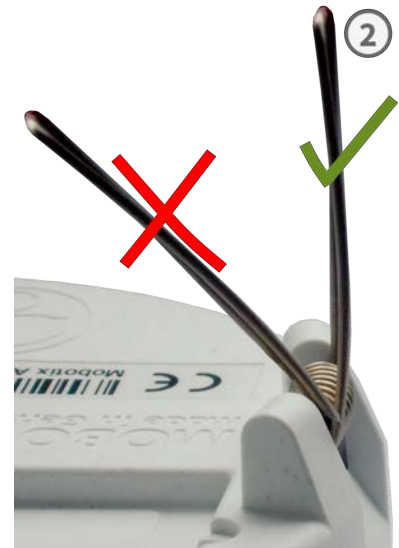

Removing the Camera from the Ceiling

Gently pull one side of the camera downward to release it, then repeat the procedure on the other side.



CAUTION!

Risk of injury! Do not allow the spring clips to snap forward ①.

1. Disconnect all cables connected to the camera (for example, the network cable and USB cable).
2. Remove the camera from the ceiling.

Surface Ceiling Installation

Preparing the Camera

1. **Remove the spring clips:** Put on safety glasses for this step. Using a small flat-head screwdriver, push against the clip as indicated by the red arrow. The clips can now be removed easily.



2. **Attach the mounting ring:** Position the mounting ring (1.5) on the camera, ensuring that the triangular mark on the mounting ring is aligned with the triangular mark on the camera.



Preparing the On-Wall Mounting Set

1. **Replace the Cable Fittings (optional):** If you route the cables through the side of the housing instead of the rear, replace one or both threaded plugs with the supplied cable fittings. Use a suitable coin to unscrew the threaded plug.



Mounting Options

-


-

2. Install the Interface Box boards (Optional):

Connect the required wires to each Interface Box board.

Insert the interface box board into the guides (red in the figure) and slide it into its final position.

Rotate the retaining tabs (blue in the figure) 90° over the board to secure it.

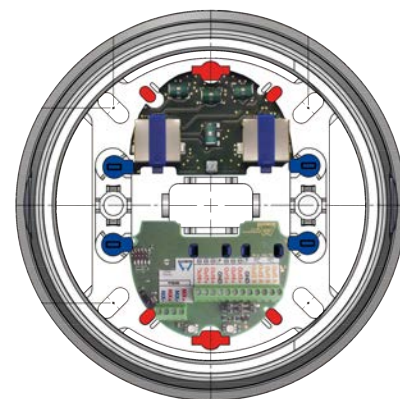

3. Connect the camera:

If interface boxes are used, connect the corresponding wires to the camera.

NOTE! For information on installing the interface boxes, refer to the corresponding documentation.

Connect the camera to the network.

If required, secure loose cables and wires using the supplied cable ties (item 1.7, see figure).



4. Insert the camera:

Position the camera with the attached mounting ring on the On-Wall Mounting Set. Ensure that no cables or wires are trapped between the mounting ring and the rim of the On-Wall Mounting Set.

Press firmly on the outer edge of the camera, as shown in the figure, until the camera audibly clicks into place. Do not press on the sensor module or the lens.

Turn the camera to the desired viewing direction.



5. Finish the installation:

Connect the camera to the power supply and complete the initial setup as described in the corresponding camera manual. Check the live image and adjust the camera, if necessary.

Removing the Camera

1. **Turn camera to the mark:** Rotate the camera until the microphone of the camera is aligned with the mark ① above the threaded plug.



2. **Firmly press down the camera:**

Press firmly on the camera at the positions indicated by the red circles until the camera tilts inward and the opposite side lifts up.



3. **Remove the camera:**

Lift the camera out of the On-Wall Mounting Set.

Disconnect the network cable and any other cables or wires connected to the camera.



Adjusting the Camera Lens

NOTE!

The camera lens is pre-focused at the factory, so this step is usually not necessary.

Adjusting the camera at the mounting position will ensure that you will see the desired field of view later on.

CAUTION!

When adjusting the image focus or the field of view of the camera, always make sure that you can see the live image of the camera on your monitor. See [Camera Software in the Browser](#), p. 49.

Adjusting and Focusing the Camera Lens

1. Focus the lens ① by turning the lens with the MultiTool module wrench [M.2](#), p. 13.
2. If required, clean the optical surfaces using a clean, lint-free cotton cloth.



Operating the Camera

Getting Started	42
Network Settings	42

Getting Started

You can use the MOBOTIX c ONE with any current browser – or with MxManagementCenter.

NOTE!
You can download MxManagementCenter free-of-charge from www.mobotix.com > [Services](#) > [Download Center](#) > [Software Downloads](#).

1. **Establish a connection to the camera:** Follow the instructions on how to access the camera as outlined in [Initial Camera Setup](#), p. 42.
2. **Configure camera:** You can use the user interface of the camera in a browser or in MxManagementCenter.

LED States

The camera LED on top of the camera body displays the following states by default:

LED status	Meaning
All off	Normal operation
Blue steady on	NurseAssist Alarm (e.g Person sitting or lying on the floor)

Network Settings

Initial Camera Setup

Check the Preconditions

- Is the camera running (check camera power LED)?
- Is the camera accessible using my current network connection?
- Do I have the necessary information for successfully running the camera on the network?
 - IP address of NTP (*Network Time Protocol*) server.
 - IP address of network gateway (if required).

Access the Camera

1. Start your web browser.
2. Access the camera using its zeroconf address:
 - Look for the factory IP address such as `10.x.y.z` on the sticker on the camera body or the packaging.
 - Enter this address in the address bar of your browser using the following syntax: `mx10-x-y-z.local`.


EXAMPLE:

Taking a factory IP address of `10.32.24.129` as an example, you would enter `mx10-32-24-129.local` in the address bar of your browser.

- Click on **Admin Menu** and enter the default access credentials (`admin/meinsm`).
3. In the **Quick Installation** dialog, select your language, then click on .



4. Continue clicking on  and do not change any settings until you reach the **Security** dialog.
Set a password for the admin user of the camera. Make sure you keep the password in a safe place.

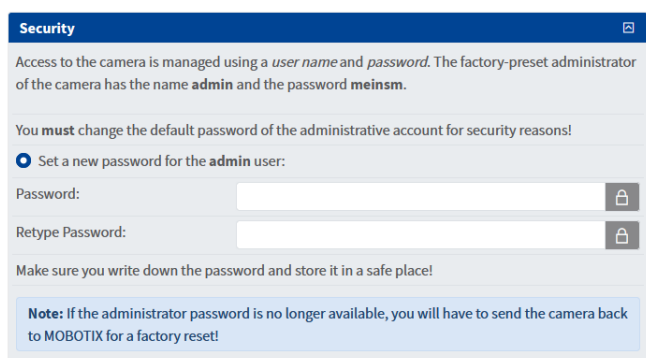


NOTE!

Make sure to record the new password in the system documentation!

Operating the Camera

Network Settings

5. Continue clicking on  and do not change any settings until you reach the **Country Settings** dialog. Check the time zone and adjust it, if necessary.

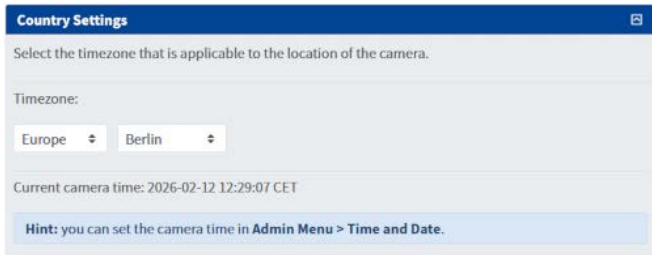

Country Settings

Select the timezone that is applicable to the location of the camera.


Timezone:

Europe Berlin

Current camera time: 2026-02-12 12:29:07 CET

Hint: you can set the camera time in Admin Menu > Time and Date.

6. Click on  and in the **Audio Settings** dialog, activate the devices that are available for this camera.

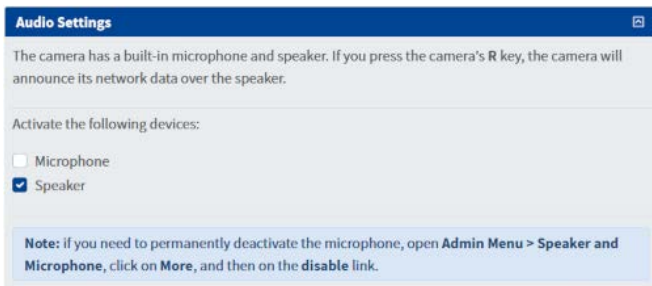

Audio Settings

The camera has a built-in microphone and speaker. If you press the camera's R key, the camera will announce its network data over the speaker.


Activate the following devices:

☐ Microphone

☒ Speaker

Note: If you need to permanently deactivate the microphone, open Admin Menu > Speaker and Microphone, click on More, and then on the disable link.

7. Click on  and in the **Camera Name** dialog, enter a descriptive camera name.

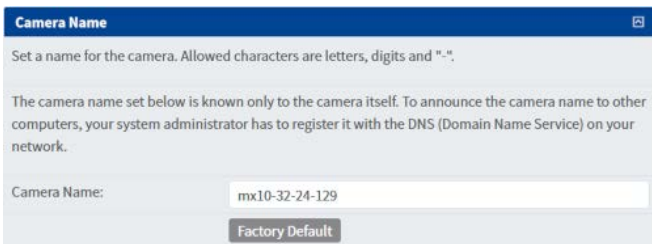

Camera Name

Set a name for the camera. Allowed characters are letters, digits and "-".

The camera name set below is known only to the camera itself. To announce the camera name to other computers, your system administrator has to register it with the DNS (Domain Name Service) on your network.

Camera Name: mx10-32-24-129

Factory Default

NOTE!

Make sure to record this camera name in the system documentation!

8. Continue clicking on  and do not change any settings until you reach the **Time Server** dialog.

Enter the IP address of your network time servers as provided by your network administrator (e.g. 192.168.1.1 ptbtime1.ptb.de; use spaces to separate multiple addresses).




Time Server

NTP Select the protocol offered by remote time servers.

192.168.1.1 ptbtime1.ptb.de Enter time server address(es).

If the time server is working properly, the LED to the right of the field turns green. A red LED indicates that the server does not work properly.

9. Click on  and review the information in the **Store Configuration** dialog. If everything is correct, print the page and include it in the system documentation.

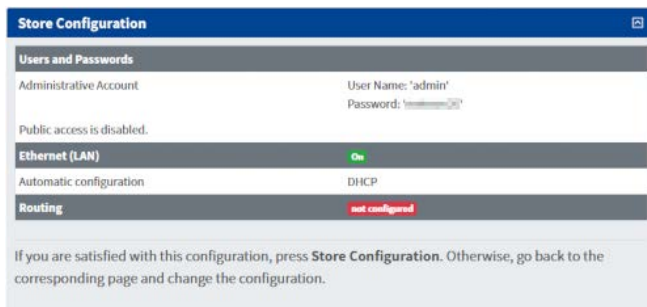


The **Store Configuration** dialog box displays the following settings:

Users and Passwords	
Administrative Account	User Name: 'admin' Password:
Public access is disabled.	
Ethernet (LAN)	
Ethernet (LAN)	On
Automatic configuration	DHCP
Routing	
Routing	not configured

If you are satisfied with this configuration, press **Store Configuration**. Otherwise, go back to the corresponding page and change the configuration.

10. Click on **Store Configuration** and then on **Reboot**.

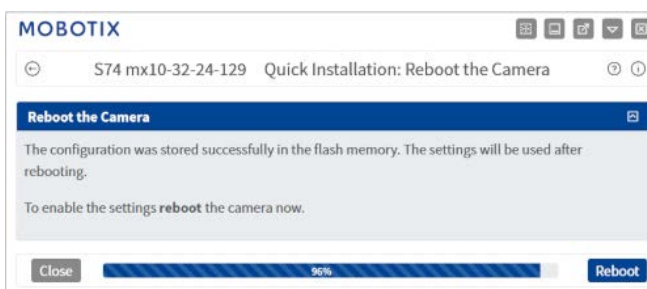

The **Reboot the Camera** dialog box displays the following information:

MOBOTIX

S74 mx10-32-24-129 Quick Installation: Reboot the Camera

The configuration was stored successfully in the flash memory. The settings will be used after rebooting.

To enable the settings **reboot** the camera now.

Close  Reboot


11. Enter the new password you entered in the **Security** dialog when prompted by the camera.

The camera will now reboot; once it is working again, you will see its live image.

Find the "Real" IP Address of the Camera

Since you are still using the `mx10-32-24-129.local` zeroconf address, you need to find out the actual IP address of the camera.

1. Click on the **Show Camera Status** icon .
2. In the **Camera Status** dialog, click on **Networking**.
 - The **Camera Name** entry shows the camera's current fully qualified domain name.
 - The **BOOTP/DHCP** status *Client running, got a lease* shows that the camera properly received an IP address.
 - The **IP Address** entry shows the camera's current address.
3. You can use either the **Camera Name** (e.g. `mx10-32-24-129.fritz.box`) or the IP address (e.g. `192.168.1.210`) to access the camera from now on.
4. Open a new browser tab and enter the address (e.g. `mx10-32-24-129.fritz.box` or `192.168.1.210`), then enter the access credentials (`admin/<your new password>`).

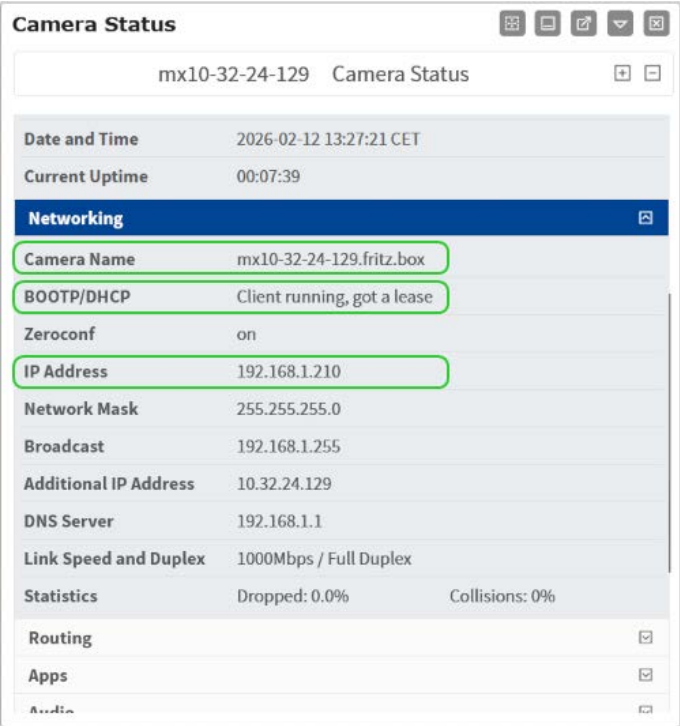

NOTE!
Make sure to record this address in the system documentation together with the camera name!

Automatic Setup using MxManagementCenter

This section describes how to use MxMC to connect the camera and configure its network settings.

MxManagementCenter is a video management software for setting up and using the entire video surveillance system that provides a range of functions for different tasks and user groups. You can download the newest release of MxManagementCenter from the MOBOTIX website (www.mobotix.com > Services > Download Center > Software Downloads, MxManagementCenter section).


Network Settings on the Camera in MxMC

When starting MxManagementCenter for the first time, the configuration wizard opens and automatically starts searching for MOBOTIX cameras. The number of detected cameras is shown next to the **Add Devices** icon.

1. Click on **Add Devices**. The cameras are displayed either in a list or as tiles. Use the List and Tile buttons to change the display mode.



The application automatically monitors and displays the operating status of all cameras using corresponding icons.

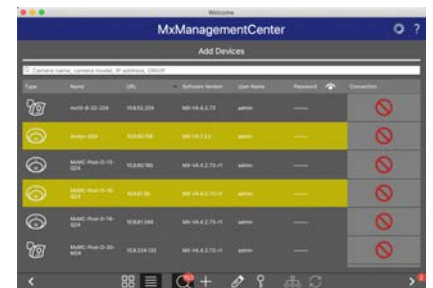

EXAMPLE:

-  The camera is not in the same subnet as the computer.
-  The user name and password of the camera are not known.

NOTE!

Using the Bonjour service ([en.wikipedia.org/wiki/Bonjour_\(software\)](https://en.wikipedia.org/wiki/Bonjour_(software))), the application finds not only MOBOTIX cameras on the same subnet, but also in other subnets. Normally, you would not be able to establish any connection to cameras in a different network or subnet.

NOTE!

This is the case, for example, if you are integrating cameras into a network without DHCP server (i.e. with fixed IP addresses) and the IP address range is different from the 10.x.x.x range supported by the cameras in addition to DHCP. MxManagementCenter can automatically configure such a camera so that it is "integrated" into your existing network.

2. Select the camera you want to set up and click on **Edit Network Settings**  at the bottom of the program window. The **Change Network Settings for Selected Devices** dialog opens.
3. Enter the IP address and the subnet mask of the selected camera.



NOTE!

The IP addresses of the other cameras are automatically incremented by 1.

4. Click on **Apply** to apply the settings.

NOTE!

For more information on this feature, please read the MxManagementCenter online help or the Tutorial (see www.mobotix.com > Services > Download Center > Documentation > Brochures & Guides > Tutorials).

Network Settings on the Camera in the Web Browser

1. Use a web browser to access the web interface of the MOBOTIX camera and enter the factory IP address (e.g. 10.16.0.99).

NOTE!

When you access the web interface for the first time, you will need to assign a new password for the admin user.

CAUTION!

If the administrator password is no longer available, the camera must be returned to MOBOTIX for a factory reset.

2. Click on the **Admin Menu** button in the user interface of the camera. The Quick Installation Wizard automatically starts after entering the access credentials of the admin user.

NOTE!

You can also run the Quick Installation Wizard later on (**Admin Menu > Network Configuration > Quick Installation**; see Reference Manual).

3. Enter the network parameters of the camera in the course of the quick installation.

NOTE!

You can also change the network parameters later on by running **Admin Menu > Network Configuration > Quick Installation**.


4. Reboot the camera to apply the network settings.

Camera Software in the Browser

Access the Camera in the Web Browser	50
Basic Settings	50

Access the Camera in the Web Browser

Once the power and network connection of the MOBOTIX have been established, you can access the interface of the camera software in a web browser.

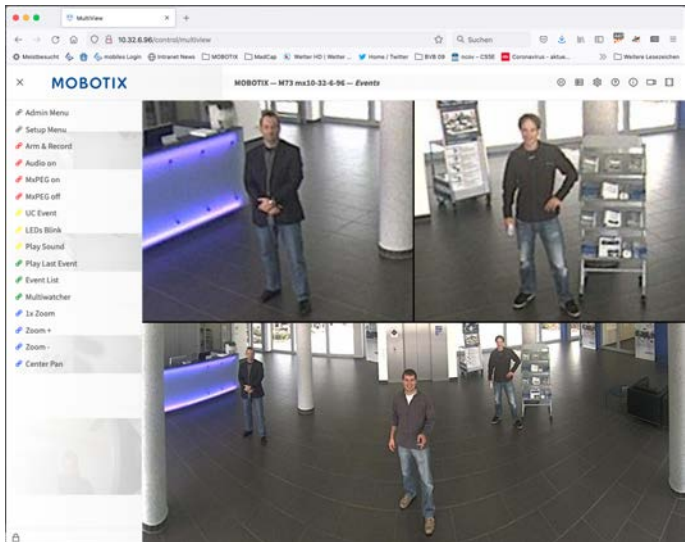

- Enter the camera's IP address in the address field of a web browser.

NOTE!

You can find the IP address of the camera, for example, in the camera housing or on the sticker on the packaging.

Basic Settings

NOTE!

You must change the password when logging in for the first time.

CAUTION!

Make sure that you store information on user names and passwords in a secure place.

If you lose the administrator password and cannot access the Administration menu, the password can only be reset at the factory. This service is subject to a service charge.

The Quick Installation Wizard will appear automatically when accessing the Administration Menu for the first time. It provides an easy method to adjust the basic camera settings to the current application scenario. For security reasons, it is highly recommended to change the default administrator password after the camera has been configured properly.

Administering the camera: You can modify the camera configuration in the Administration Menu or the Setup Menu:

- **Admin Menu:** This menu contains the basic configuration dialogs of the camera (e.g. passwords, interfaces, software update).

- **Setup Menu:** This menu contains the dialogs for configuring the image, event and recording parameters. Some of these settings can be changed using the corresponding Quick Controls in the Live screen.

NOTE!

For more information, consult the Reference Manual of the camera (see www.mobotix.com > **Services** > **Download Center** > **Marketing & Documentation** > **User Manuals**).

Maintenance

Replacing the microSD Card	54
Cleaning the Camera	54

Replacing the microSD Card

CAUTION!

Risk of equipment damage and data loss.

- Before removing the microSD card, disable recording and reboot the camera.
- Disconnect the camera from the power supply.
- Do not touch the circuit board while replacing the microSD card.
- Ensure that the microSD card is not write-protected.

1. **Deactivate storage:** If storage on microSD card is still activated, deactivate it in the camera's web interface: **Admin Menu > Storage on External File Server / Flash Device**, then reboot the camera.
2. Disconnect the camera's power supply.
3. **Open the housing:** (see [Removing the Back Plate, p. 28](#)).
4. **Remove the microSD card:** Gently push the microSD card into the slot to release it from the push lock. Then pull it out with tweezers.



5. **Insert microSD card:** Carefully insert the new microSD card into the slot using tweezers and press it in lightly until it clicks into place.
6. **Close the housing:** (see [Attaching the Back Plate, p. 29](#)).
7. **Activate storage:**
 - Format a new microSD card as outlined in the camera's *Storage on External File Server / Flash Device* online help topic.
 - If the microSD card already is formatted with MxFFS, you can activate storage in **Admin Menu > Storage on External File Server / Flash Device**. After rebooting the camera, recording will automatically resume.
8. **Reboot the camera.**

Cleaning the Camera

To ensure safe and effective cleaning and disinfection of the smart sensor c ONE NurseAssist in care environments, it is important to consider both the integrity of the equipment and the health and safety of patients and staff. Given the variety of materials used in these devices and the need to ensure effective disinfection to prevent the spread of infection,

this document is intended as a guide to help to select the appropriate cleaning agents and procedures for your c ONE NurseAssist devices, considering both material compatibility and hygiene requirements in care environments.

Cleaning and Disinfection Instructions

This section describes the proper procedure for cleaning and disinfecting the surfaces of the c ONE NurseAssist surveillance camera in order to ensure long-term functionality and prevent damage to sensitive components.

NOTE!

Perform cleaning and disinfection only by qualified personnel in accordance with this documentation.

General Requirements

Use only **soft microfiber cloths** for cleaning.

Do not use abrasive or rough cloths that may scratch or damage the surface.

Do not spray the device directly with cleaning or disinfecting agents.

CAUTION!

Prevent liquid ingress

Liquid ingress may permanently damage the audio components.

- Do not use a wet cloth.
- Use only the minimum amount of cleaning agent required for proper cleaning.
- Prevent cleaning agents from entering the microphone and speaker openings.
- Avoid direct spraying of the device.

CAUTION!

Prevent functional impairment of the sensor

Residues may attract dust and restrict the sensor's field of view.

- Prevent cleaning agent residues from remaining on the surface.
- Prevent dust or particles from accumulating on the lens cover.

Cleaning Procedure

1. Lightly moisten a soft microfiber cloth with a suitable cleaning or disinfecting agent.
2. Gently wipe all external surfaces without applying excessive pressure.
3. Ensure that no liquid enters any device openings (microphone, speaker).
4. Wipe the device thoroughly with a dry microfiber cloth after cleaning to remove all residues.

Post-Cleaning Requirements

Proper drying minimizes chemical stress on audio components and prevents dust accumulation that may impair sensor performance (e.g., restricted field of view due to contamination of the lens cover).

- Ensure that no visible residue remains on the surface.
- Ensure that all surfaces are completely dry.

Approved Cleaning Agents and Disinfectants

The following list contains a range of approved cleaning and disinfecting agents that are suitable for ensuring the longevity and performance of your devices.

These products have been specifically selected for their compatibility with the device's surface materials and promise minimal impact with an exposure time of at least 60 hours.

Agent	Compatibility
Isopropanol (Isopropyl alcohol; IPA) 70%	Compatible at 1.0% concentration
Ethanol (Ethyl Alcohol)	Compatible at 0.5% concentration
Saline Solution 10%	Compatible at 1.0% concentration

Incompatible Cleaning Agents

Do not use the following substances as they can damage the surfaces or impair the effectiveness of the disinfection:

- Methyl Ethyl Ketone (MEK)
- Organic compounds containing lipid hydrocarbons, including fatty acid derivatives
- DEHP (Di(2-ethylhexyl) phthalate)
- Bleach (Sodium hypochlorite solution)
- Cidex glutaraldehyde-based disinfectants
- Virex organic ammonium chloride-based disinfectants
- Betadine microbicide; povidone-iodine solution
- Hydrogen peroxide



EN_07/26

MOBOTIX AG • Am Stundenstein 2 • D-67722 Winnweiler • Tel.: +49 6302 9816-103 • sales@mobotix.com • www.mobotix.com
MOBOTIX is a trademark of MOBOTIX AG registered in the European Union, the U.S.A., and in other countries. Subject to change without notice. MOBOTIX do not assume any liability for technical or editorial errors or omissions contained herein. All rights reserved. © MOBOTIX AG 2019